# ADC® 2200 Advantage™ Fingertip Pulse Oximeter

# **Directions for Use**





## ADC® Fingertip Pulse Oximeter

Thank you for purchasing an ADC ADvantage™ Fingertip Pulse Oximeter. We're proud of the care and quality that goes into the manufacture of every product that bears our name. The ultra-portable Advantage™ 2200 will give you information about oxygen saturation (the amount of oxygen in the blood) and pulse rate at your fingertip. The 2200 is easy to use and needs no routine maintenance except battery replacement. This User's Guide explains how to use and care for your Advantage™ 2200

#### Contents of this Package

- Advantage<sup>™</sup> 2200
- Two "AAA" batteries

Lanvard

User Guide

#### Intended use

The Advantage<sup>™</sup> 2200 is intended to measure blood oxygen saturation (%SpO<sub>2</sub>) – the amount of oxygen in your blood – and pulse rate. It is designed for use on fingers (not the thumb) with a thickness of 8mm to 20mm (.31" to .79"), this is the distance between the fingernail (top) and finger pad (bottom). The index finger is most recommended. This device is intended for sport and aviation purposes only.

#### Contraindications:

- The patient suffers from significant levels of dysfunctional hemoglobins (such as carbonxy-hemoglobin or methemoglobin).
- Intravascular dyes such as indocyanine green or methylene blue have been injected into the patient.
- Used in the presence of high ambient light (ie, direct sunlight). Shield the sensor area
  with a surgical towel if necessary.
- There is excessive patient movement.
- The patient experiences venous pulsations.
- The patient has hypotension, severe vasoconstriction, severe anemia, or hypothermia.
- The patient is in cardiac arrest or is in shock.
- Patients have fingernail polish or false fingernails as they may cause inaccurate Sp02 readings.

### Symbol Definitions


The following symbols are associated with your Advantage™ 2200

Symbol	Definition	
<b>†</b>	The equipment type is BF	
	Refer to user manual before use	
% SpOa	Hemoglobin saturation	
●PR BPM	Heart Rate (BPM) Beats per Minute	

Symbol	Definition	
\text{\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\ext{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\exitin}\$}}}}}}}}}}}}}}}}}}}}}}}}}}}}}}}}}}	Low Power Indication	
**	Manufacturing Date	
SpO <sub>2</sub>	Not for continuous monitoring	

### General Warnings 🗥





**WARNING:** Explosion hazard: Do not use the pulse oximeter in an explosive (oxygen enriched) environment.

CAUTION: Only a healthcare professional is qualified to interpret SpO₂ measurements. This device is NOT intended to replace regular medical checkups.

**CAUTION:** It is recommended that your physician review your procedure for using this device.

**CAUTION:** Excessive movement of the Advantage™ 2200 during measurement may cause inaccurate readings. Limit finger movement as much as possible when using the device.

CAUTION: The Advantage™ 2200 is not intended for continuous monitoring.

CAUTION: Do not place the Advantage™ 2200 on the same hand/arm when using a blood pressure monitor.


CAUTION: The Advantage™ 2200 has NO alarms. It will not sound if the amount of oxygen in your blood is low or if the pulse rate is too high or too low.



CAUTION: Do not immerse the Advantage™ 2200 in liquid or clean with agents that are not listed in this User's Guide.

CAUTION: Any of the following conditions may reduce the performance of the Advantage™ 2200:

- Very bright or flickering light
- Weak pulse
- Low hemoglobin
- Arterial catheters
- Nail polish and/or artificial nails
- Any tests recently performed on you that required the injection of intravascular dyes



CAUTION: Batteries can leak or explode if used or disposed of improperly. Remove the battery if the Advantage™ 2200 will not be used for more than 30 days.

CAUTION: Do not use the Advantage™ 2200 outside the specified operating and storage temperature ranges.

**CAUTION:** Do not use the Advantage™ 2200 for more than 30 minutes without relocating the device to another finger.

**CAUTION:** Do not tamper with the Advantage™ 2200.

CAUTION: Radios, cell phones or other similar devices may affect the Advantage™ 2200 and should be kept at least 7 feet away from the device.

**CAUTION:** Use in emergency vehicles with communication systems may affect the accuracy of the Advantage™ 2200.

CAUTION: Field strengths from fixed transmitters (radio, phone base stations, AM/FM radio or TV broadcast towers) may affect the accuracy of the Advantage™ 2200.


CAUTION: Follow local ordinances and recycling instructions regarding disposal or recycling of the Advantage™ 2200 including batteries.

CAUTION: The Advantage™ 2200 is a precision electronic instrument and must be serviced by ADC's service department.

WARNING: This product may contain a chemical known to the state of California to cause cancer, birth defects, or other reproductive harm.

#### Battery Installation (figure 1)

- 1. Slide off battery cover in direction of arrow.
- 2. Put the two AAA batteries into battery compartment by observing correct polarity.
- 3. Slide the battery cover on by reversing Step #1.

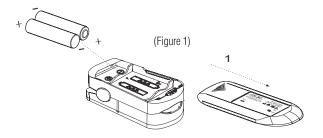


#### Note:

- Battery polarity should be observed to prevent damage to the device.
- When battery is low, the battery indicator symbol on the display will flash. Replace low battery
  as soon as possible. Remove battery if the device will not be used for more than 30 days.


### Strap Installation (figure 2)

- 1. Thread thinner end of the strap through the loop.
- 2. Thread thicker end of the strap through the threaded end before pulling it tightly.

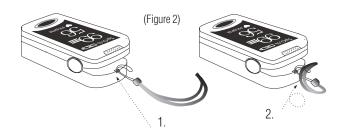

#### Operation Instructions (figure 3)

- 1. Hold the Advantage™ 2200 with the display screen facing toward you as shown in Figure 3. Gently squeeze the hinged end and insert one finger into the device fully. Release hinged end to allow device to clamp down onto finger. Be sure finger is fully inserted. (When your finger is inserted into the device, your nail surface must be facing the same side as the display.)
- 2. Press the power button on the front panel once.
- 3. Remain still while taking a measurement and avoid applying pressure to the clamped device while in use
- 4. The device will display a reading once it has had a moment to begin measurement.




#### Note:

- The rubber inside the Oximeter that touches the finger maybe cleaned with alcohol.
- For best results, keep the Advantage™ 2200 at heart or chest level.
- The index (pointer) finger is recommended.
- While on the finger, do not press the Advantage™ 2200 against any surface and do not squeeze it or hold the device.
- The internal spring provides the correct pressure. Additional pressure may affect readings.

### Reading Your Results

After measurement begins, you will see three pieces of information displayed on your pulse oximeter:

- A pulse bar graph display corresponding with your pulse beat will be shown. The height of the bar graph shows your pulse strength.
- Your pulse rate will be displayed as **BPM** or beats per minute.
- The amount of oxygen in your blood will be displayed as SpO<sub>2</sub>%.



### Changing Directions of the Display

When you first power on the unit, the display will orient it with the numbers facing the person wearing the device. The display can be re-orientated to face the other direction, if desired.

 To change the direction of the display, press the power button while the unit is displaying a reading.

**Note:** By default, the unit will always display the readout facing the wearer.

#### Maintenance and Storage

- 1. When the low power indicator comes on, you must replace the batteries.
- The surface of the pulse oximeter that comes into contact with your finger should be kept clean.
- 3. When storing the pulse oximeter for more than 30 days, remove the batteries.
- 4. When storing the pulse oximeter, ensure that the temperature is between -13°F to 158°F (-25°C to 70°C) with a relative humidity greater than or equal to 93%.
- Store the pulse oximeter in a dry environment. Exposure to moisture may decrease the lifespan of your device.
- 6. Batteries should be disposed of in accordance with local and state laws.

#### Cleaning the Pulse Oximeter

Clean the rubber touching the finger inside of the device with a soft dampened cloth with 70% isopropyl alcohol, and clean the test finger using alcohol before and after each test. Do not pour or spray any liquids onto the Oximeter, and do not allow any liquids to enter any openings in the device. Allow the device to dry thoroughly before reusing.

## Detailed Description of Product Functions

1. Display Type: LED		Low power indication:
2. SpO <sub>2</sub> : Measuremen	='	Battery Life: Two AAA 1.5V, 1200mAh Alkaline. Could continuously operate for 18 hrs.
range: Accuracy:	70-100% 70%-100%, ±2%; 69% no definition.	5. Dimensions: Length: 2.19" (5.5cm) Width: 1.13" (2.9cm)
3. Pulse Rate: Measure range: 30bpm~250bpm Accuracy: 30~99BPM, ±2BPM;		Height: 1" (2.5cm) Weight: 1.76oz. (50g) (including two AAA batteries)
Pulse Intensi	100bpm~250bpm ty: Bar Graph Indicator	<b>6. Environment Requirements:</b> Operation Temperature:
4. Power Requirements:		41°F-104°F (5°C - 40°C) Storage Temperature:
Two (2) AAA alkaline Batteries		-13°F to 158°F (-25°C to 70°C) Ambient Humidity:
Power consu Less than	•	Operation: 15%~93% no condensation in operation Storage: 93% no condensation in storage/transport

## Troubleshooting

Problems	Possible reason(s)	Solution(s)
SpO <sub>2</sub> or pulse rate cannot be shown normally	Finger is not inserted correctly     Oxyhemoglobin value is too low to be measured	Re-insert/re-position finger     Ensure that sensor is clean and not blocked     Try taking a reading on a different finger or warm your finger by rubbing
SpO <sub>2</sub> or pulse rate is shown unstably	Finger might not be inserted deep enough     Excessive movement during measurement	Re-insert/re-position finger     Remain still during measurement
The Oximeter cannot be powered on	Low battery strength     Batteries installed incorrectly     The Oximeter might be damaged	Replace batteries     Reinstall the batteries     Contact warranty center for service
Display suddenly powers off.	The product is automatically powered off when no signal is detected for longer than 8 seconds     Low battery strength	Re-insert/re-position finger     Replace the batteries
"Error7"	Low power     Oximeter is damaged	Replace batteries     Contact warranty center for service

### Limited Warranty

American Diagnostic Corporation (ADC®) warrants its products against defects in materials and workmanship under normal use and service as follows:

- 1. Warranty service extends to the original retail purchaser only and commences with the date of delivery.
- 2. Your Pulse Oximeter is warranted for one (1) year from date of purchase (all parts).

What is Covered: Replacement of parts, and labor.

What is Not Covered: Transportation charges to and from ADC<sup>®</sup>. Damages caused by abuse, misuse, accident, or negligence. Incidental, special, or consequential damages. Some states do not allow the exclusion or limitation of incidental, special, or consequential damages, so this limitation may not apply to you.

**To Obtain Warranty Service:** Send item(s) postage paid to ADC®, Attn: Repair Dept., 55 Commerce Dr., Hauppauge, NY 11788. Please include your name and address, phone no., proof of purchase, and a brief note explaining the problem.

**Implied Warranty:** Any implied warranty shall be limited in duration to the terms of this warranty and in no case beyond the original selling price (except where prohibited by law).

This warranty gives you specific legal rights and you may have other rights which vary from state to state

**Declaration:** This product complies with the IEC60601-1-2 standard. The user-contacting materials are non-toxic and comply with ISO10993-1, ISO10993-5 and ISO10993-10.

# Guidance and manufacturer's declaration - electromagnetic emissions for all EQUIPMENT and SYSTEMS

Guidance and manufacturer's declaration - electromagnetic emission

The *Pulse Oximeter* is intended for use in the electromagnetic environment specified below. The customer or the user of the *Pulse Oximeter* should assure that it is used in such an environment

Emission Test	Compliance	Electromagnetic Environment Guidance
RF emissions CISPR 11	Group 1	The Pulse Oximeter uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The Pulse Oximeter is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.



Beijing Choice

Electronic Technology Co., Ltd. Room 4104, No. A12 Yuquan Road Haidian District, 100043 Beijing, P.R. China

EC REP

Shanghai International Holding Corp. GmbH (Europe) EiffestraBe 80, 20537



Distributed by: ADC® 55 Commerce Drive Hauppauge, NY 11788

Inspected in the U.S.A.

Made in China
tel: 631-273-9600
1-800-232-2670
fax: 631-273-9659
www.adctoday.com

IB p/n 93-2200-00 rev 6

Printed in China